




FORMATO DE DATOS MENSUAL DE LOS EQUIPOS SECUENCIALES (PARTISOL) PM10 CORT SEPTIEMBRE 2-17

Fecha dd/mm/aa	Numero de filtro	W Filt limp (g)	W Filt usado (g)	W test inic (g)	W test final (g)	PTP (g)	Volumen (m3 ref)	Concentración (Ug/m3 ref) con	Act Start Time	Set Stop Time	Ilo	Ihi	Bplo	Bphi	ICA
02/09/2010	P0000055	0,15116	0,15200	0,79033	0,79042	0,0007500	24,0480	31	00:00	00:00	0	50	0	54	28,88
05/09/2010	P0000056	0,14922	0,14996	0,79033	0,79042	0,0006500	24,0480	27	00:00	00:00	0	50	0	54	25,03
08/09/2010	P0000057	0,14885	0,14995	0,79033	0,79042	0,0010100	24,0480	42	00:00	00:00	0	50	0	54	38,89
10/09/2010	P0000058	0,14915	0,14978	0,79033	0,79042	0,0005400	24,0480	22	07:00	07:00	0	50	0	54	20,79
14/09/2010	P0000059	0,15230	0,15319	0,79033	0,79042	0,0008000	24,0480	33	00:00	00:00	0	50	0	54	30,80
17/09/2010	P0000065	0,14870	0,14970	0,79033	0,79042	0,0009100	24,0480	38	00:00	00:00	0	50	0	54	35,04

\*Día sin carro

Concentración

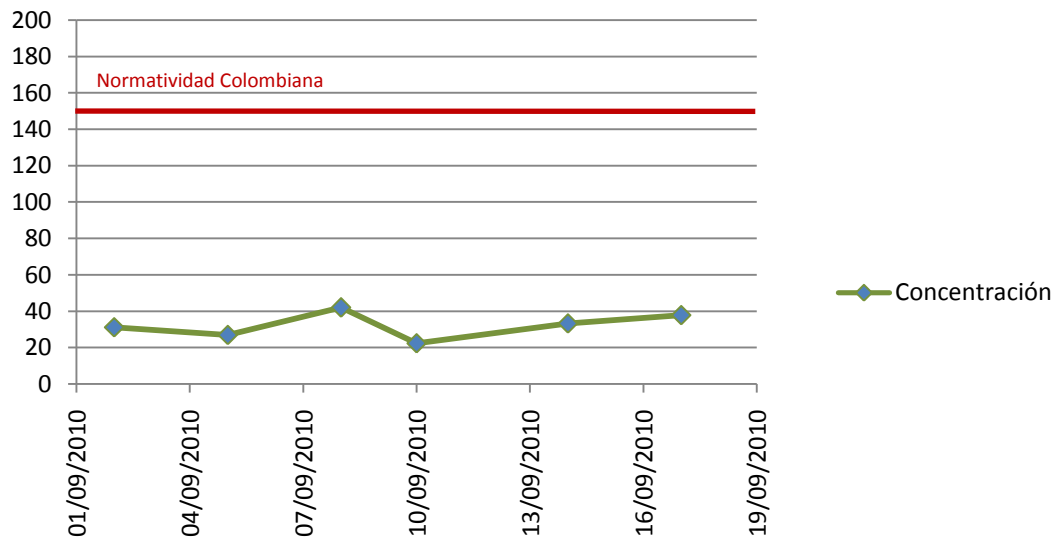

ICA

