




FORMATO DE DATOS MENSUAL DE LOS EQUIPOS SECUENCIALES (PARTISOL) PM10 PAY DICIEMBRE 2 - 29

Fecha dd/mm/aa	Numero de filtro	W Filt limp (g)	W Filt usado (g)	W test inic (g)	W test final (g)	PTP (g)	Volumen (m3 ref)	Concentrac iòn (Ug/m3 ref) con Total Min	Act Start Time	Set Stop Time	llo	lhi	Bplo	Bphi	ICA
02/12/2010	P0000090	0,15002	0,15054	0,79043	0,79046	0,0004900	24,0480	20	00:00	00:00	0	50	0	54	18,87
05/12/2010	P0000091	0,15015	0,15063	0,79043	0,79046	0,0004500	24,0480	19	00:00	00:00	0	50	0	54	17,33
11/12/2010	P0000092	0,15002	0,15042	0,79043	0,79046	0,0003700	24,0480	15	00:00	00:00	0	50	0	54	14,25
14/12/2010	P0000093	0,15001	0,15048	0,79043	0,79046	0,0004420	24,0480	18	00:00	00:00	0	50	0	54	17,02
17/12/2010	P0000094	0,15010	0,15059	0,79043	0,79046	0,0004600	24,0480	19	00:00	00:00	0	50	0	54	17,71
23/12/2010	P0000095	0,15006	0,15061	0,79043	0,79046	0,0005200	24,0480	22	00:00	00:00	0	50	0	54	20,02
26/12/2010	P0000096	0,14999	0,15063	0,79043	0,79046	0,0006100	24,0480	25	00:00	00:00	0	50	0	54	23,49
29/12/2010	P0000097	0,15001	0,15061	0,79043	0,79046	0,0005700	24,0480	24	00:00	00:00	0	50	0	54	21,95

Concentración

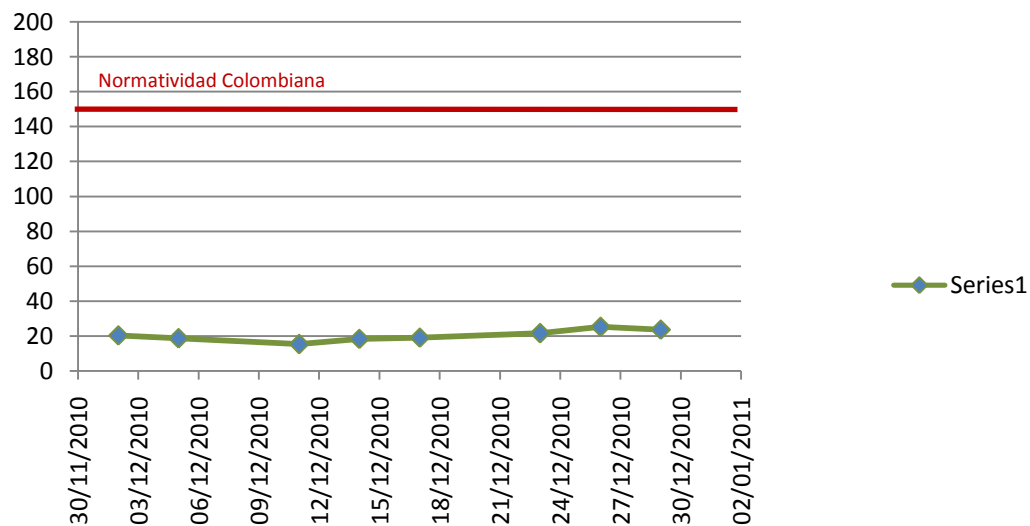

ICA

